


# Certificate

**Polymer Technology Systems Inc (PTS Diagnostics)**

using

**A1cNow+, A1cNow SELF CHECK**

participated in the IFCC HbA1c Certification Programme to demonstrate traceability to the IFCC Reference Measurement Procedure and performed as shown below.

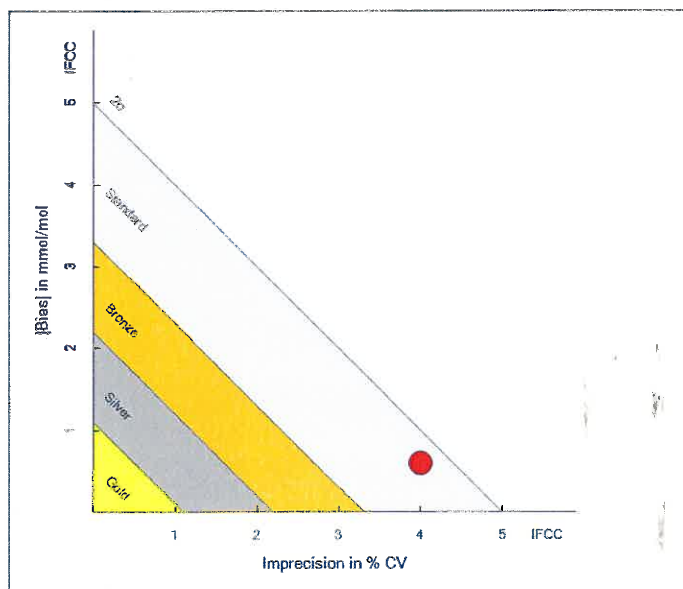

Total Error =	4.6	mmol/mol
Bias =	-0.6	mmol/mol
Imprecision =	4.0	%
Grade =	Standard	

Criteria derived from the IFCC model for Quality Targets HbA1c (Clin Chem 2015;61 : 752-59)

Date of Certification : 01 January 2020

Date of Expiry : 01 January 2021



IFCC Network Coordinator  
Dr. C.W. Weykamp