


Certificate

Polymer Technology Systems Inc (PTS Diagnostics)

using

A1cNow+, A1cNow Self Check

participated in the IFCC HbA1c Certification Programme to demonstrate traceability to the IFCC Reference Measurement Procedure and performed as shown below.

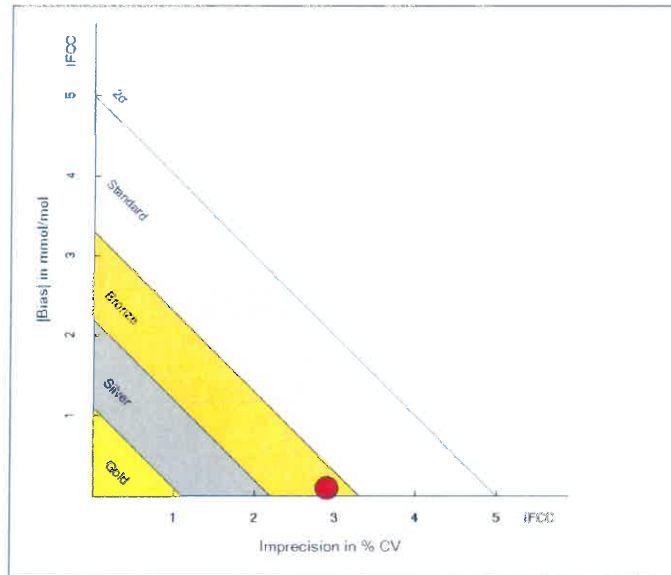


Total Error =	3.0	mmol/mol
Bias =	+0.1	mmol/mol
Imprecision =	2.9	%
Grade =	Bronze	

Criteria derived from the IFCC model for Quality Targets HbA1c (Clin Chem 2015;61 : 752-59)

Date of Certification : 01 January 2021

Date of Expiry : 01 January 2022


 IFCC Network Coordinator
 C. Siebelder